


# Airflows Within a Class II Biological Safety Cabinet

Clean/filtered air supplied to work area

Dirty room air enters at 100 fpm

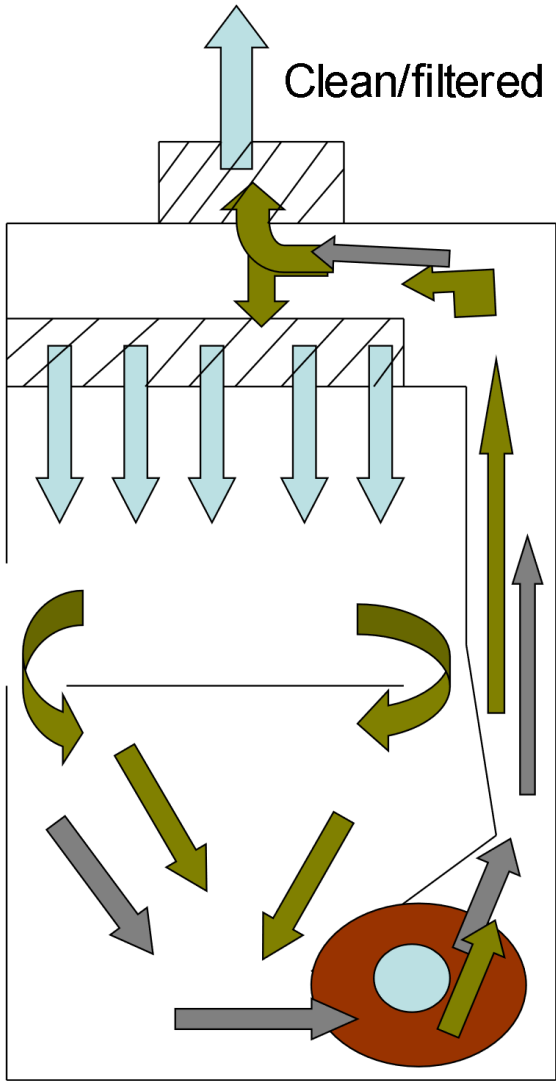

Clean/filtered air exhausted back to room

Supply & Exhaust HEPA filters

Contaminated air in work area is directed down below work surface through front and rear grills

Blower directing room and "dirty" air up through HEPA filters